



Safety and accuracy of neonatal continuous glucose monitoring

メタデータ	言語: English 出版者: 日本小児科学会 公開日: 2024-11-11 キーワード (Ja): キーワード (En): Accuracy, Blood glucose, Neonate, Safety, Continuous glucose monitoring 作成者: Ohishi, Akira, Ueno, Daizo, Fujita, Tomoka, Segawa, Yuki, Yamamoto, Takuya, Fujisawa, Yasuko, Iijima, Shigeo メールアドレス: 所属:
URL	http://hdl.handle.net/10271/0002000243

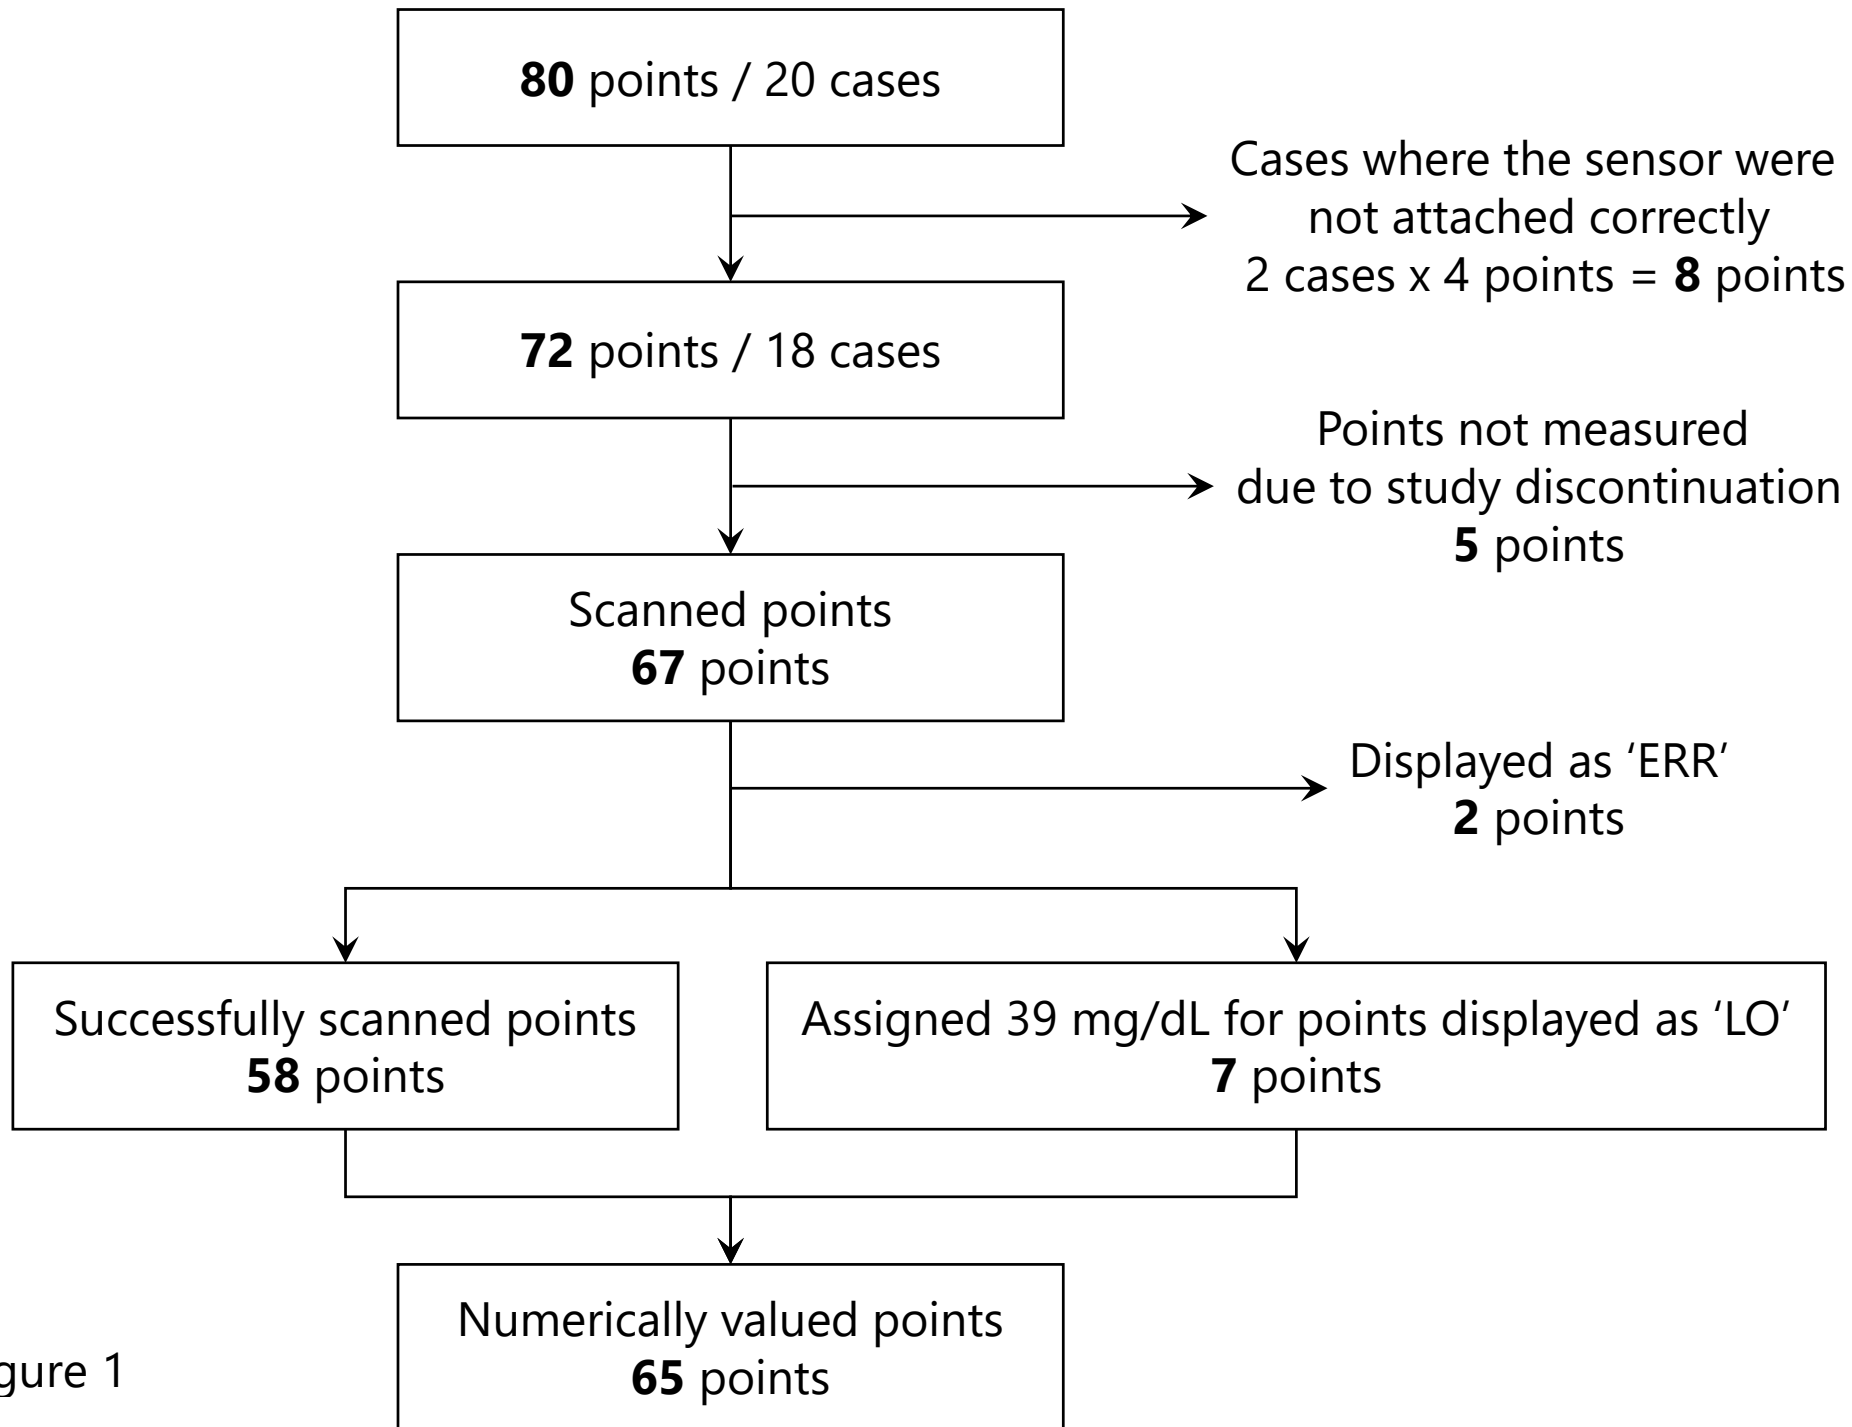


Figure 1

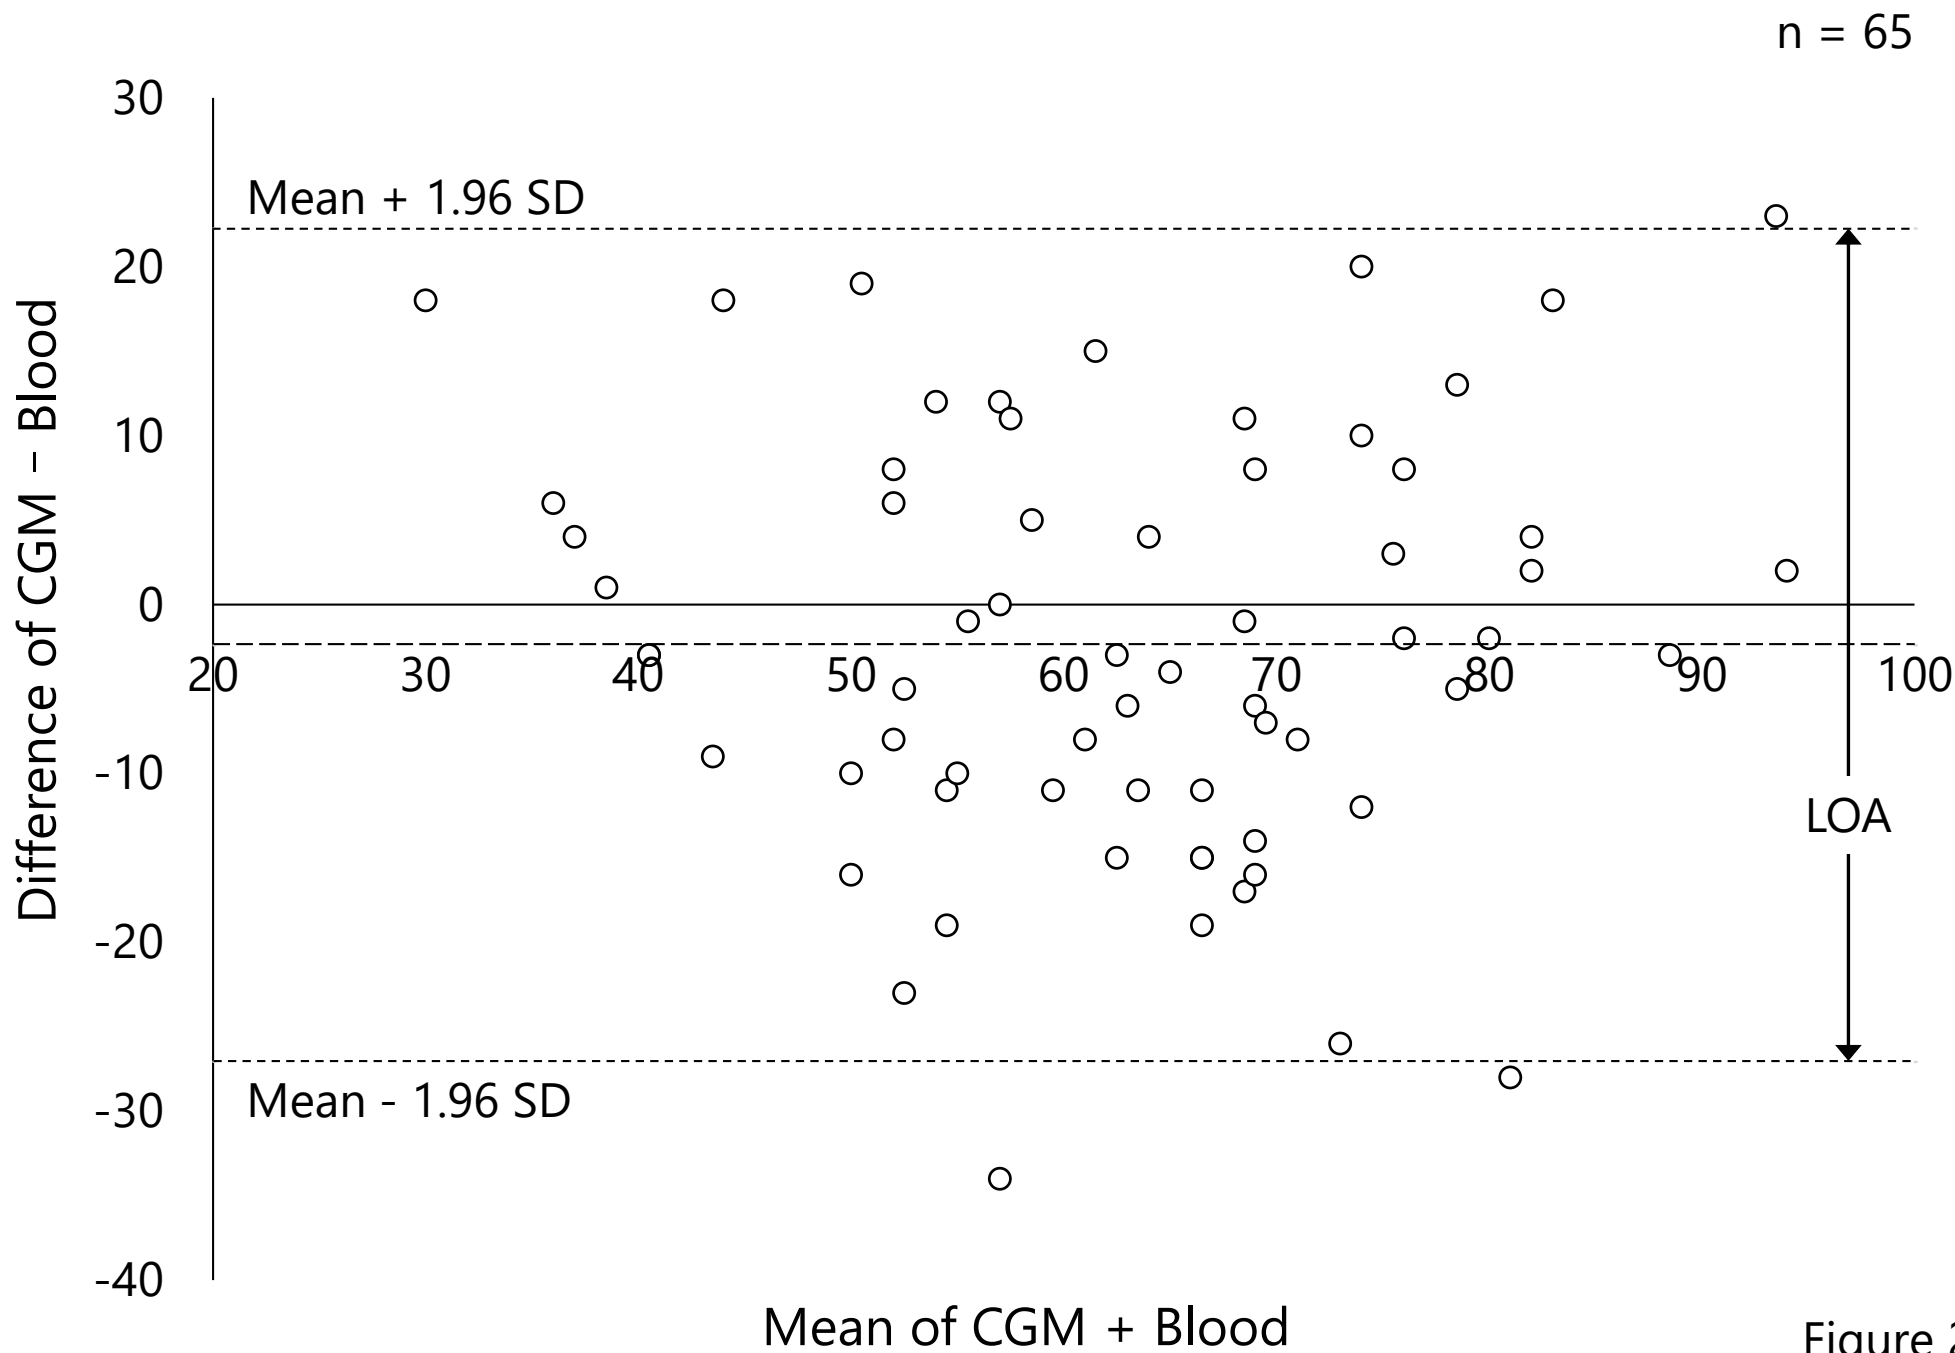


Figure 2

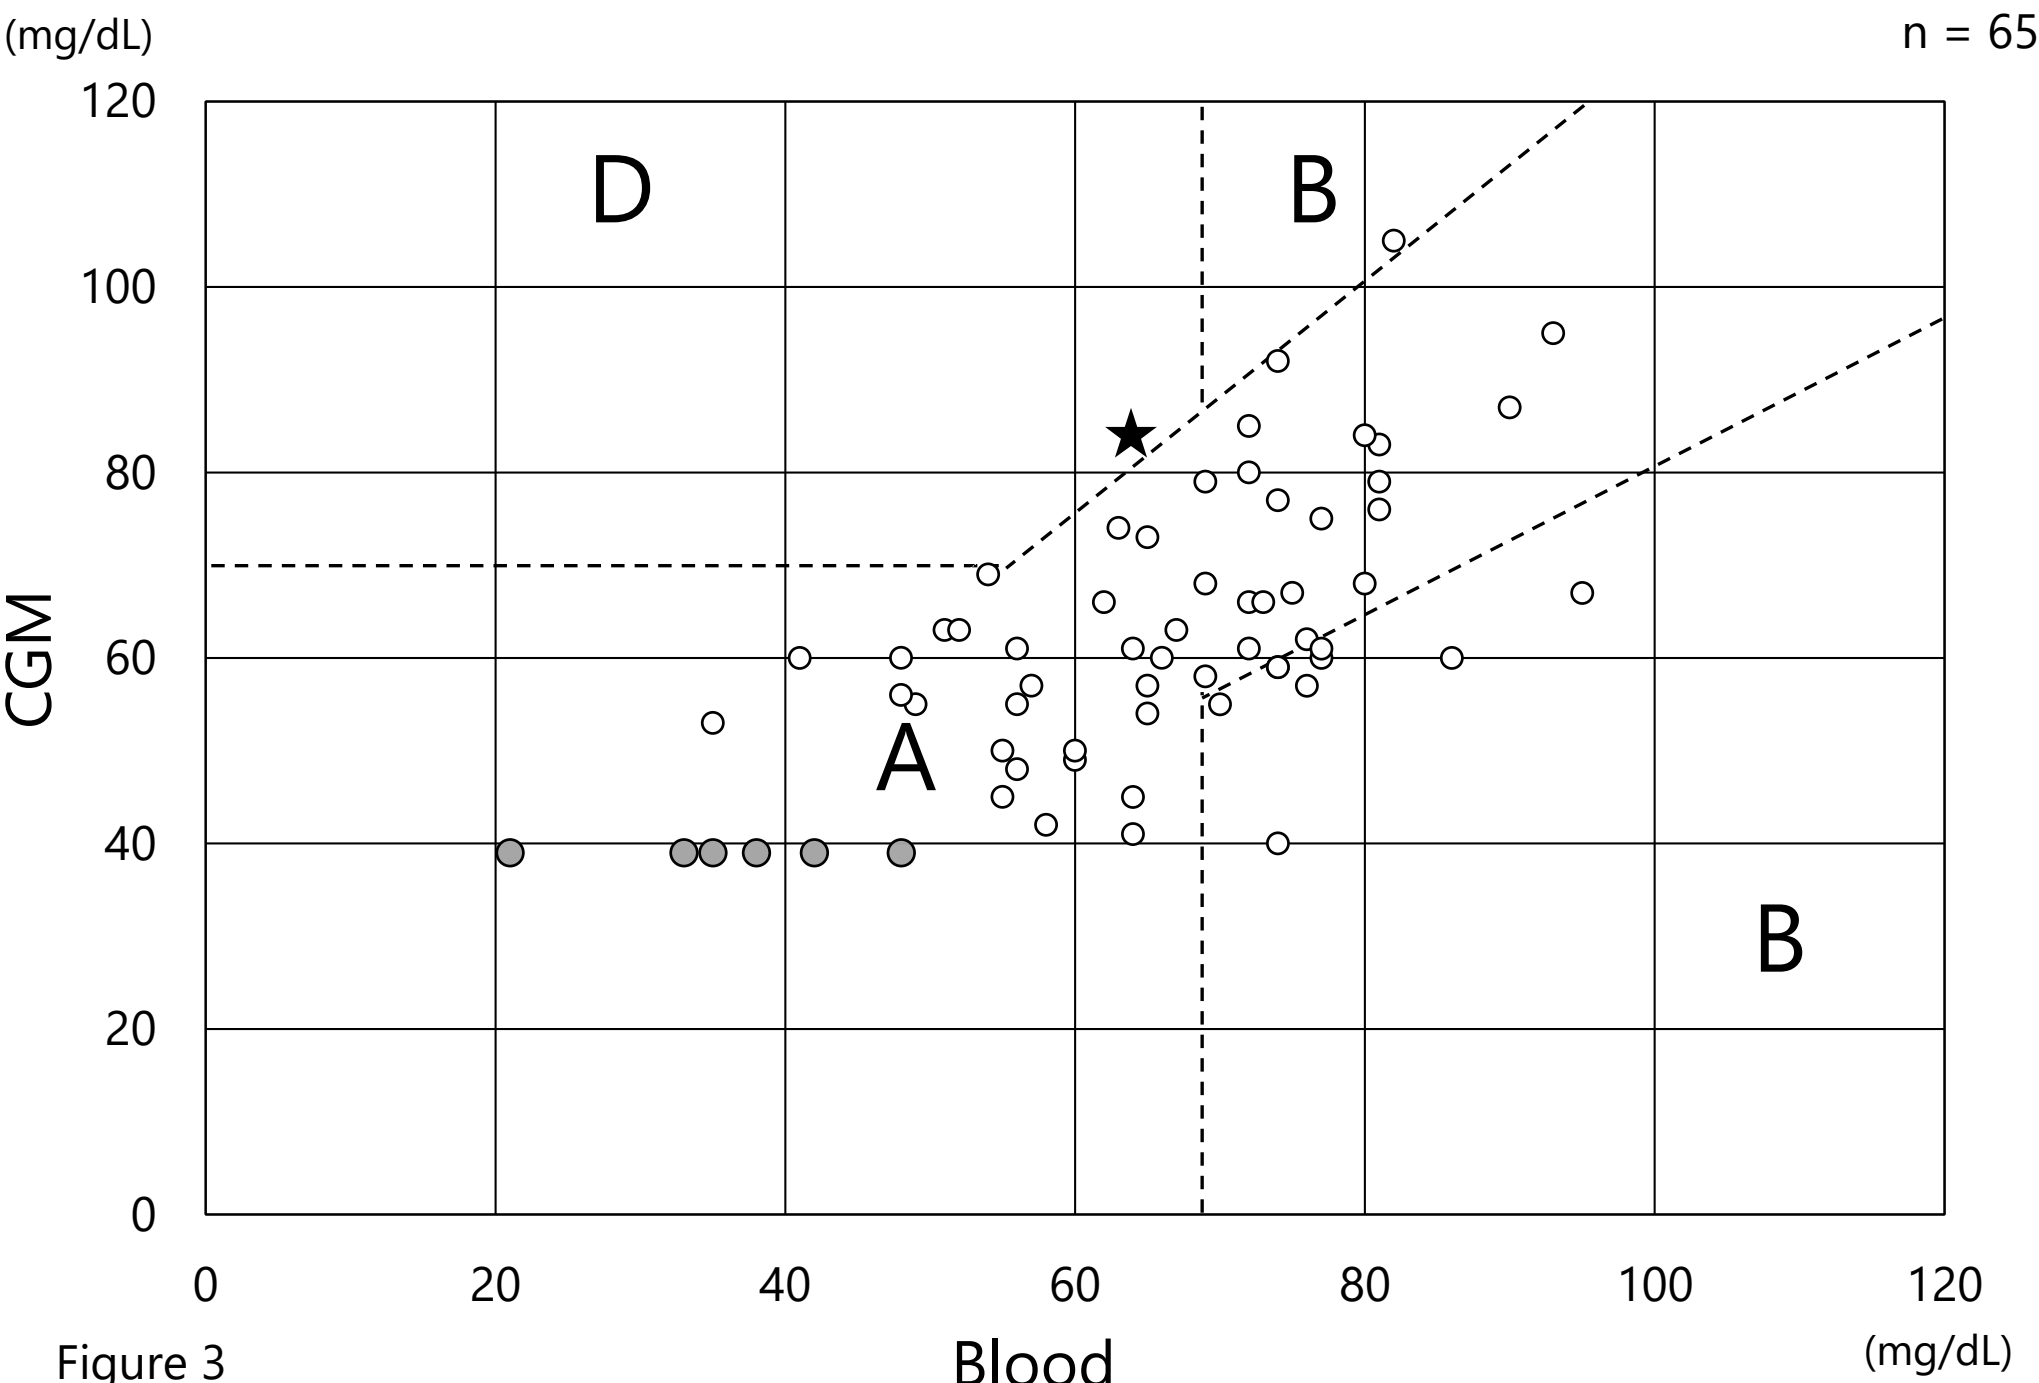


Figure 3

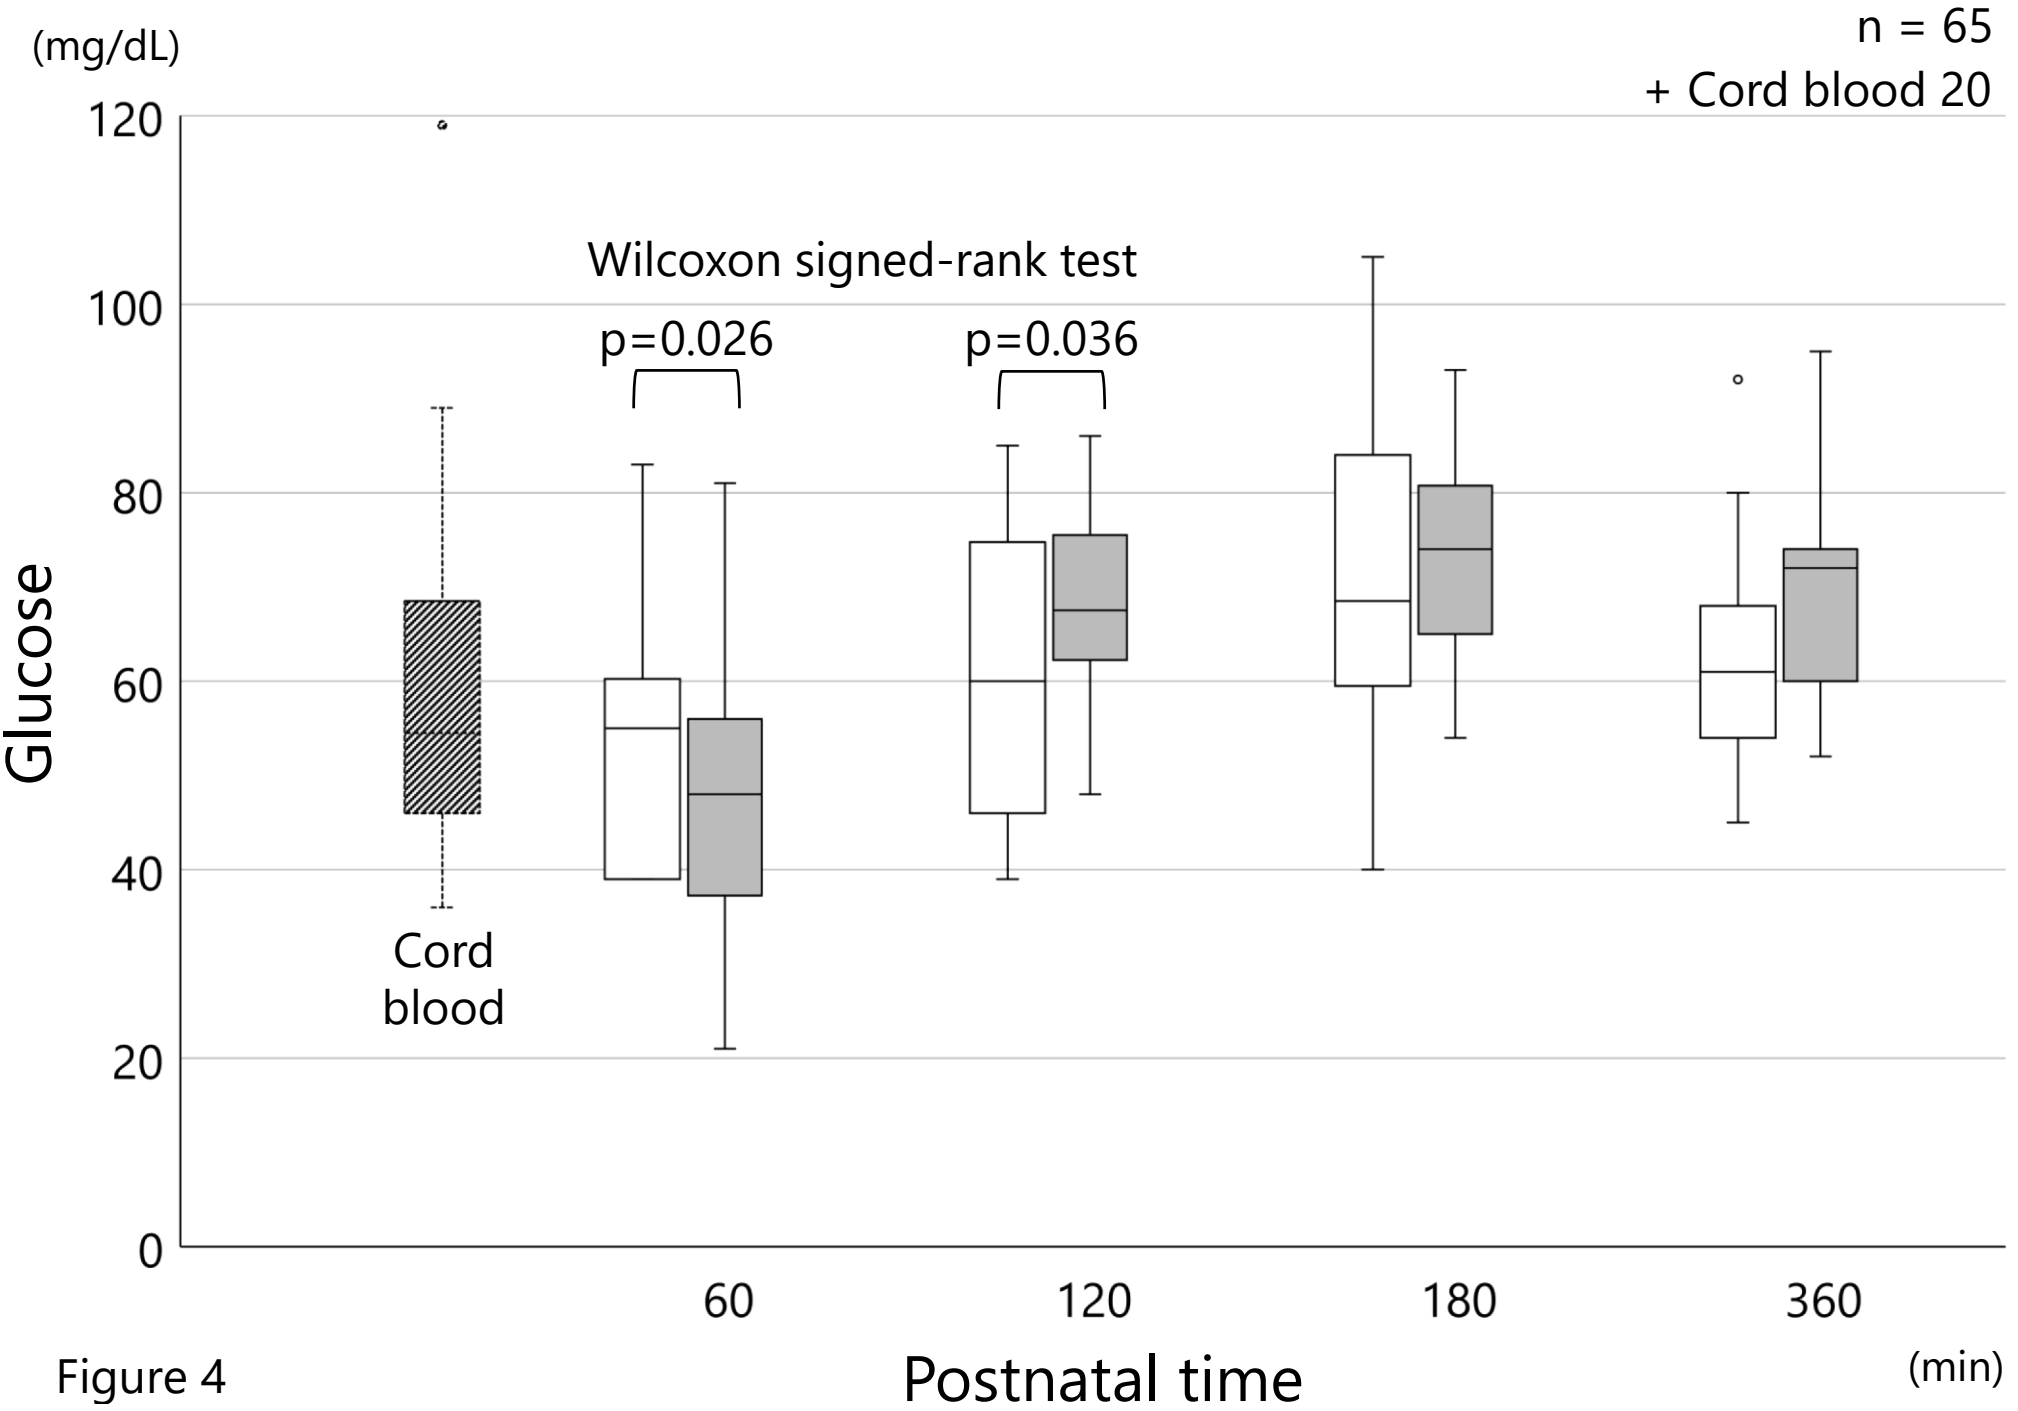


Figure 4